



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
10/772,500	02/05/2004	Barry Davignon	10707/016	5664

7590 04/10/2007
David H. Badger, Esq.
BRINKS HOFER GILSON & LIONE
One Indiana Square, Suite 1600
Indianapolis, IN 46204

EXAMINER

MENDOZA, MICHAEL G

ART UNIT	PAPER NUMBER
----------	--------------

3734

SHORTENED STATUTORY PERIOD OF RESPONSE	MAIL DATE	DELIVERY MODE
3 MONTHS	04/10/2007	PAPER

Please find below and/or attached an Office communication concerning this application or proceeding.

If NO period for reply is specified above, the maximum statutory period will apply and will expire 6 MONTHS from the mailing date of this communication.

ED

Office Action Summary	Application No. 10/772,500	Applicant(s) DAVIGNON, BARRY	
	Examiner Michael G. Mendoza	Art Unit 3734	

-- The MAILING DATE of this communication appears on the cover sheet with the correspondence address --

Period for Reply

A SHORTENED STATUTORY PERIOD FOR REPLY IS SET TO EXPIRE 3 MONTH(S) OR THIRTY (30) DAYS, WHICHEVER IS LONGER, FROM THE MAILING DATE OF THIS COMMUNICATION.

- Extensions of time may be available under the provisions of 37 CFR 1.136(a). In no event, however, may a reply be timely filed after SIX (6) MONTHS from the mailing date of this communication.
- If NO period for reply is specified above, the maximum statutory period will apply and will expire SIX (6) MONTHS from the mailing date of this communication.
- Failure to reply within the set or extended period for reply will, by statute, cause the application to become ABANDONED (35 U.S.C. § 133). Any reply received by the Office later than three months after the mailing date of this communication, even if timely filed, may reduce any earned patent term adjustment. See 37 CFR 1.704(b).

Status

- 1) ☒ Responsive to communication(s) filed on 05 February 2004.
- 2a) ☐ This action is **FINAL**. 2b) ☒ This action is non-final.
- 3) ☐ Since this application is in condition for allowance except for formal matters, prosecution as to the merits is closed in accordance with the practice under *Ex parte Quayle*, 1935 C.D. 11, 453 O.G. 213.

Disposition of Claims

- 4) ☒ Claim(s) 1-29 is/are pending in the application.
- 4a) Of the above claim(s) _____ is/are withdrawn from consideration.
- 5) ☒ Claim(s) 18-29 is/are allowed.
- 6) ☒ Claim(s) 1,3-6 and 8-10 is/are rejected.
- 7) ☒ Claim(s) 2, 7, and 11-17 is/are objected to.
- 8) ☐ Claim(s) _____ are subject to restriction and/or election requirement.

Application Papers

- 9) ☐ The specification is objected to by the Examiner.
- 10) ☐ The drawing(s) filed on _____ is/are: a) ☐ accepted or b) ☐ objected to by the Examiner.
 Applicant may not request that any objection to the drawing(s) be held in abeyance. See 37 CFR 1.85(a).
 Replacement drawing sheet(s) including the correction is required if the drawing(s) is objected to. See 37 CFR 1.121(d).
- 11) ☐ The oath or declaration is objected to by the Examiner. Note the attached Office Action or form PTO-152.

Priority under 35 U.S.C. § 119

- 12) ☐ Acknowledgment is made of a claim for foreign priority under 35 U.S.C. § 119(a)-(d) or (f).
- a) ☐ All b) ☐ Some c) ☐ None of:
1. ☐ Certified copies of the priority documents have been received.
 2. ☐ Certified copies of the priority documents have been received in Application No. _____.
 3. ☐ Copies of the certified copies of the priority documents have been received in this National Stage application from the International Bureau (PCT Rule 17.2(a)).
- * See the attached detailed Office action for a list of the certified copies not received.

Attachment(s)

- | | |
|---|---|
| 1) <input type="checkbox"/> Notice of References Cited (PTO-892) | 4) <input type="checkbox"/> Interview Summary (PTO-413)
Paper No(s)/Mail Date. _____ |
| 2) <input type="checkbox"/> Notice of Draftsperson's Patent Drawing Review (PTO-948) | 5) <input type="checkbox"/> Notice of Informal Patent Application |
| 3) <input checked="" type="checkbox"/> Information Disclosure Statement(s) (PTO/SB/08)
Paper No(s)/Mail Date <u>2/5/2004</u> . | 6) <input type="checkbox"/> Other: _____ |

DETAILED ACTION

Claim Rejections - 35 USC § 112

1. The following is a quotation of the second paragraph of 35 U.S.C. 112:

The specification shall conclude with one or more claims particularly pointing out and distinctly claiming the subject matter which the applicant regards as his invention.
2. Claim 9 is rejected under 35 U.S.C. 112, second paragraph, as being indefinite for failing to particularly point out and distinctly claim the subject matter which applicant regards as the invention.
3. It is unclear and vague as to what the radius of curvature of as a human eyeball equates to. The radius of curvature and vary from and infant to and adult. The radius of curvature can also vary do to impaired eyes, i.e., and eye with an astigmatism.

Claim Rejections - 35 USC § 102

4. The following is a quotation of the appropriate paragraphs of 35 U.S.C. 102 that form the basis for the rejections under this section made in this Office action:

A person shall be entitled to a patent unless –

(b) the invention was patented or described in a printed publication in this or a foreign country or in public use or on sale in this country, more than one year prior to the date of application for patent in the United States.

5. Claims 1, 3, 8, and 10 are rejected under 35 U.S.C. 102(b) as being anticipated by Fukuda 4345601.
6. Kukuda teaches an apparatus for suturing tissue, comprising: a curved suture needle; and a suture control apparatus comprising a pair of needle guides separated by a space and a locator surface in the space between the needle guides for engagement with tissue to receive a suture, said needle guides providing substantially the same radius of curvature as the radius of curvature of said suture needle, the space between

Art Unit: 3734

said needle guides and the location of said locator surface being selected to define the depth of the suture through tissue pressed against the locator surface in the space between the needle guides when the curved suture needle is passed through the needle guides and the tissue; wherein the needle guides are curved and formed by lengths of tubing; wherein the locator surface is curved; and wherein the pair of needle guides and locator surface are carried by a handle.

FIG. 1

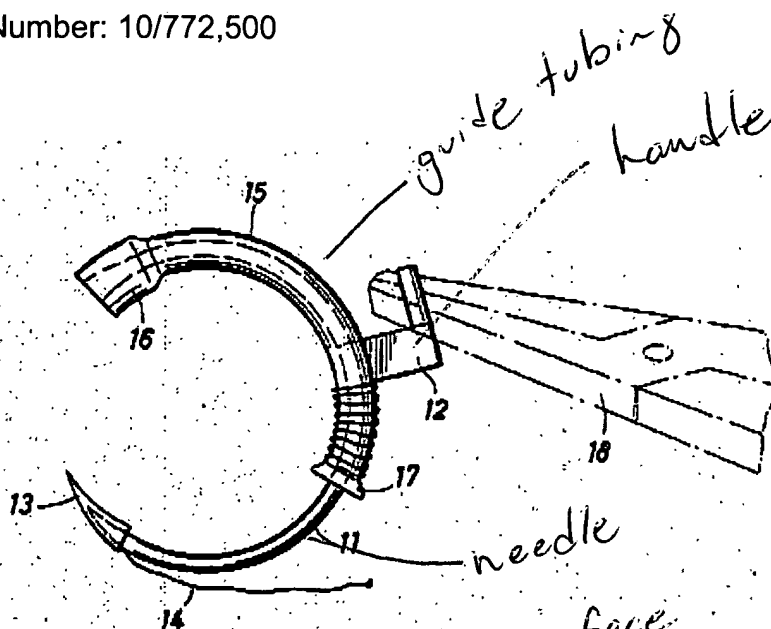


FIG. 2

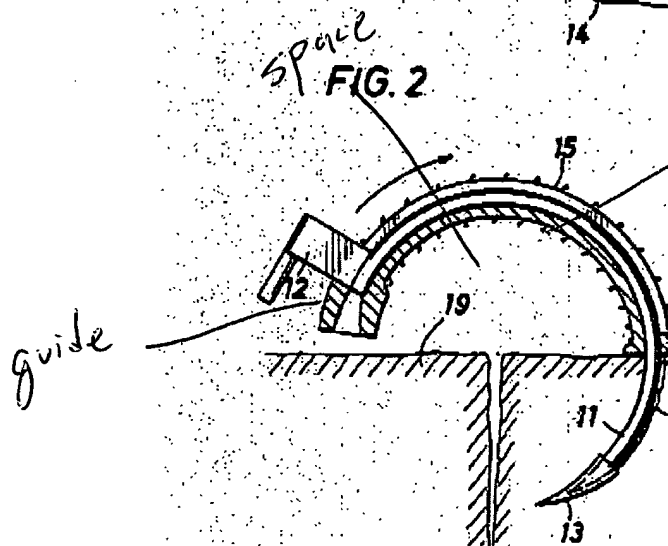


FIG. 3


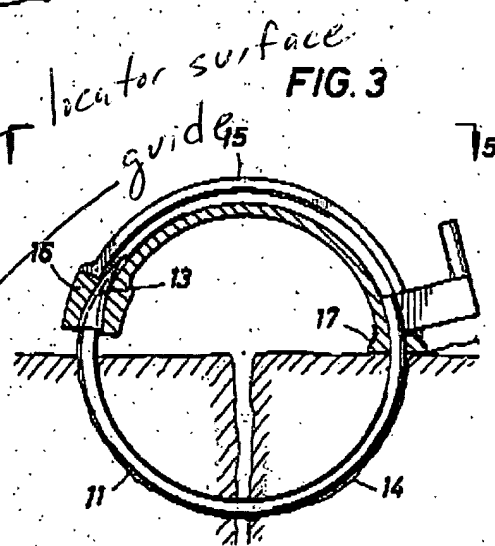


FIG. 4

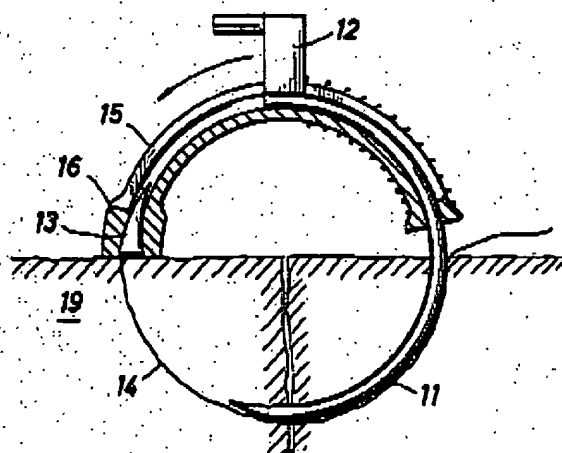

Art Unit: 3734

Claim Rejections - 35 USC § 103

7. The following is a quotation of 35 U.S.C. 103(a) which forms the basis for all obviousness rejections set forth in this Office action:

(a) A patent may not be obtained though the invention is not identically disclosed or described as set forth in section 102 of this title, if the differences between the subject matter sought to be patented and the prior art are such that the subject matter as a whole would have been obvious at the time the invention was made to a person having ordinary skill in the art to which said subject matter pertains. Patentability shall not be negated by the manner in which the invention was made.

8. Claims 4-6 are rejected under 35 U.S.C. 103(a) as being unpatentable over Fukuda.

9. Fukuda fails to teach a non-circular/polygonal/triangular needle guides.

However, it would have been obvious to one having ordinary skill in the art at the time the invention was made to use the claimed shapes because the shape of the needle guide is a mere design choice and that any shape would perform equally well.

Allowable Subject Matter

10. Claims 18-29 are allowable over the prior art of record.

11. Claims 2, 7, and 11-17 are objected to as being dependent upon a rejected base claim, but would be allowable if rewritten in independent form including all of the limitations of the base claim and any intervening claims.

Contacts

Any inquiry concerning this communication or earlier communications from the examiner should be directed to Michael G. Mendoza whose telephone number is (571) 272-4698. The examiner can normally be reached on Mon.-Fri. 9:00 a.m. - 5:00 p.m..

Art Unit: 3734

If attempts to reach the examiner by telephone are unsuccessful, the examiner's supervisor, Michael Hayes can be reached on (571) 272-4959. The fax phone number for the organization where this application or proceeding is assigned is 571-273-8300.

Information regarding the status of an application may be obtained from the Patent Application Information Retrieval (PAIR) system. Status information for published applications may be obtained from either Private PAIR or Public PAIR. Status information for unpublished applications is available through Private PAIR only. For more information about the PAIR system, see <http://pair-direct.uspto.gov>. Should you have questions on access to the Private PAIR system, contact the Electronic Business Center (EBC) at 866-217-9197 (toll-free). If you would like assistance from a USPTO Customer Service Representative or access to the automated information system, call 800-786-9199 (IN USA OR CANADA) or 571-272-1000.



MM



MICHAEL J. HAYES
SUPERVISORY PATENT EXAMINER